Design-in guidelines for XENSIV™ PAS CO2 gas sensors

Ensuring ideal operation in various applications

About this document

Scope and purpose

This application note is designed to support system designers in optimizing the environmental and mechanical integration of Infineon's XENSIV™ PAS CO2 gas sensors. The document provides detailed guidance on the implementation of these sensors, with a focus on the PASCO2V01 [1] and PASCO2V15 [2] models. Additionally, it outlines recommended application scenarios for the sensor, and offers practical advice on ensuring ideal operation in various applications.

Intended audience

The intended audiences for this document are design engineers, technicians, and developers of electronic systems interested in integrating the XENSIV™ PAS CO2 gas sensors into their designs.

Table of contents

About this document **1**
Table of contents **2**
1 Introduction to XENSIV™ PAS CO2 module **3**
2 Working principles of XENSIV™ PAS CO2 ..... **4**
3 Recommendations to ensure an ideal operation **5**
3.1 Proper coupling with the ambient conditions 5
3.2 Several preventive measures should be considered 5
3.3 Minimize noise in 12 V supply line 7
3.4 Assembly instructions 7
4 Typical application scenarios **10**
4.1 Influence of acoustic signal within a speaker 10
4.2 Influence of vibration within an air purifier 10
4.3 Sensor coverage within an indoor environment 11
References **13**
Revision history **14**
Disclaimer **15**

1 Introduction to XENSIV™ PAS CO2 module

As shown in Figure 1, XENSIV™ PAS CO2 comprises a gas measuring cell with an infrared (IR) emitter, a high-SNR microphone as the acoustic detector, and an XMC™ microcontroller for data processing. The diffuser port on the top side of the measuring cell allows for efficient gas exchange while maintaining dust protection. The sensor module allows for integration via surface mount soldering via the pads on the bottom side of its PCB. All the key components are developed in-house, ensuring the highest quality and performance. However, proper implementation of the sensor in the application environment is essential to achieve the best sensor performance.

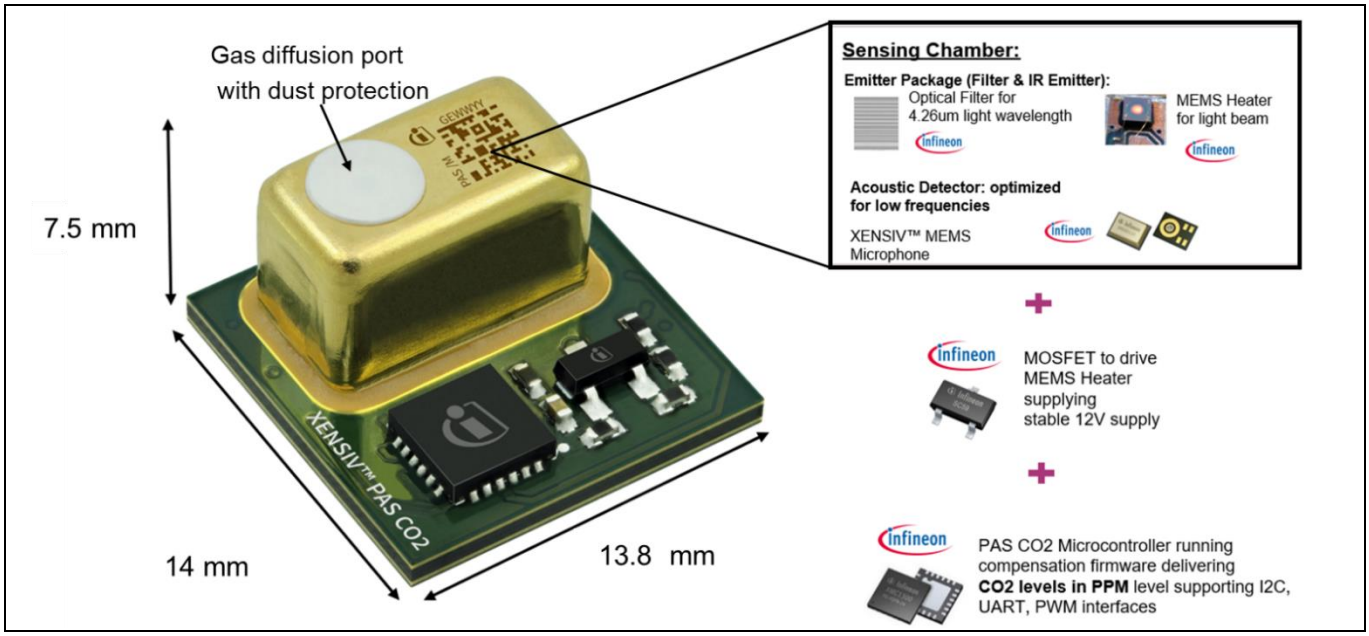

Figure 1 XENSIV™ PAS CO2 gas sensor (PASCO2V01)

All the key components of XENSIV™ PAS CO2 are developed in-house to ensure best-in-class quality of the sensor.

2 Working principles of XENSIV™ PAS CO2

Before the recommendations, here is a recap of the working principles of photoacoustic spectroscopy (PAS). As shown in Figure 2, the emitter IR light source (black body radiator) emits a wide spectrum, and the optical filter only allows 4.2 µm wavelength. CO2 molecules inside the chamber absorb light at 4.2 µm wavelength and are excited. The IR emitter needs to be chopped at a certain frequency to ensure the CO2 molecules create enough acoustic pressure change inside the cavity, which is then detected by the acoustic detector at the resonance frequency.

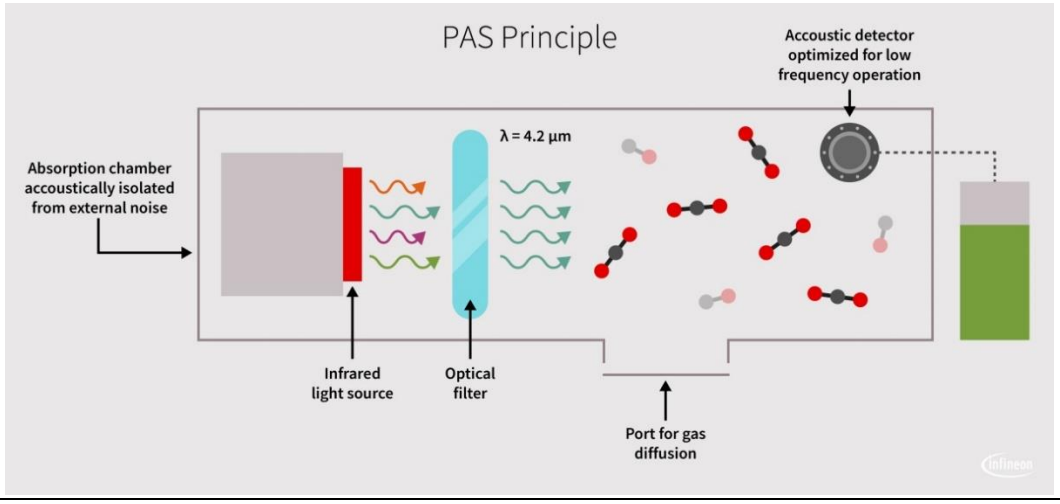

Figure 2 Working principles of photo acoustic spectroscopy

Three essential building blocks dictate if the sensor will perform well or not in the application environment:

- **Building block 1:** Proper CO2 molecule diffusion via the gas port
- **Building block 2:** Selective 4.2 µm light from the emitter
- **Building block 3:** Acoustic pressure change only due to CO2 molecule excitation is detected by the microphone

In the following section, these three building blocks will be addressed with proper recommendations to ensure good performance of the sensor in the application system.

3 Recommendations to ensure an ideal operation

3.1 Proper coupling with the ambient conditions

As discussed in the previous section, for proper operation the CO2 molecules need to be diffused properly within the sensor cavity. To ensure proper coupling, the following conditions must be met:

- The device needs to be positioned in such a way that the diffusion of CO2 molecules can happen easily, with a large enough opening. The recommended opening is at least 14 mm x 14 mm
- CO2 concentration should not be trapped inside the application chamber cavity. The back volume of the application chamber cavity should be around 3.89 cm^3 (1.8 cm x 1.8 cm x 1.2 cm)

An example of a good environmental coupling is shown in Figure 3.

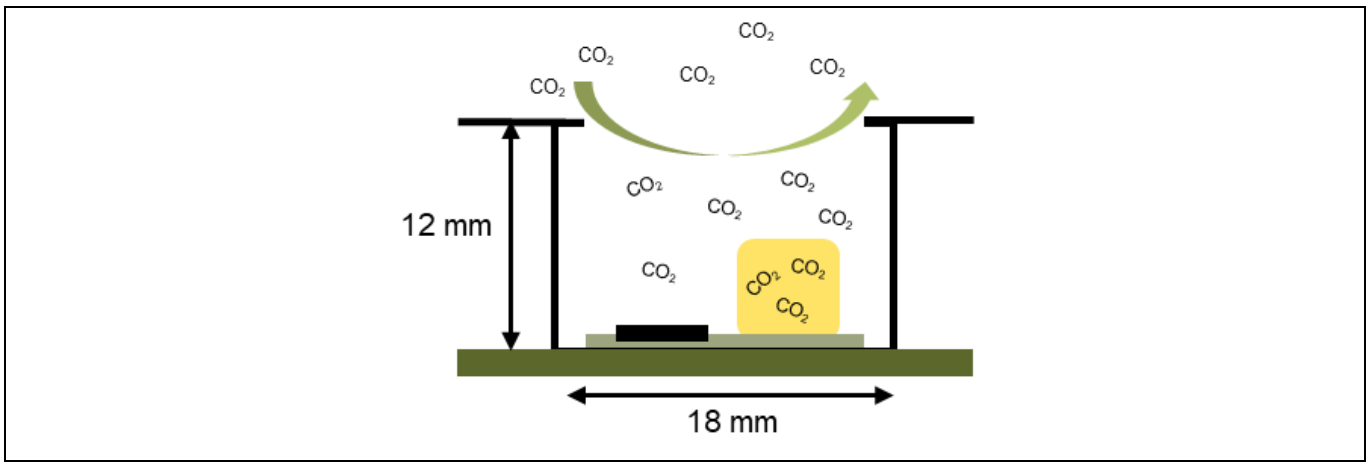

Figure 3 Example of ideal coupling with the ambient conditions

3.2 Several preventive measures should be considered

In addition to good coupling with the environment, the following preventive measure should also be considered.

- **Protection from direct air flow:** The sensor should not be placed directly in the flow. Depending on the flow, the pressure within the application cavity might alter, which could introduce additional errors due to random pressure variation
- **Isolation from a temperature source:** Within the operating range of 0°C to 50°C, the XENSIV™ PAS CO2 sensor largely compensates for the impact of temperature. The built-in XMC™ temperature sensor is used for this compensation. However, if there is a heat source next to the sensor, the device will not experience the ambient temperature, rather it will only consider the board temperature. Therefore, the compensation scheme might be disturbed if the heat source influences the temperature measurement by the XMC™. Consequently, for ideal operating conditions, it is recommended that the sensor remains isolated from adjacent heat sources
- **Isolation from vibration:** The detector of the PAS technology is a MEMS microphone, which quantifies small pressure changes within the gas cavity. Low-frequency vibrations may create a similar pressure change, and the sensor may consider this small pressure change as the real CO2 concentration change. Therefore, it is recommended to ensure that the sensor remains isolated from a direct vibration source. However, if it will not be possible to ensure vibration isolation, it is recommended to identify the vibration source first and position the sensor in such a way that the vibration comes from the x-direction of the sensor, as shown in Figure 4. Additionally, during continuous mode and fast sampling rate operation it is

recommended to enable the denoiser filter (stepwise reactive IIR), which further minimizes the impact of vibrations.

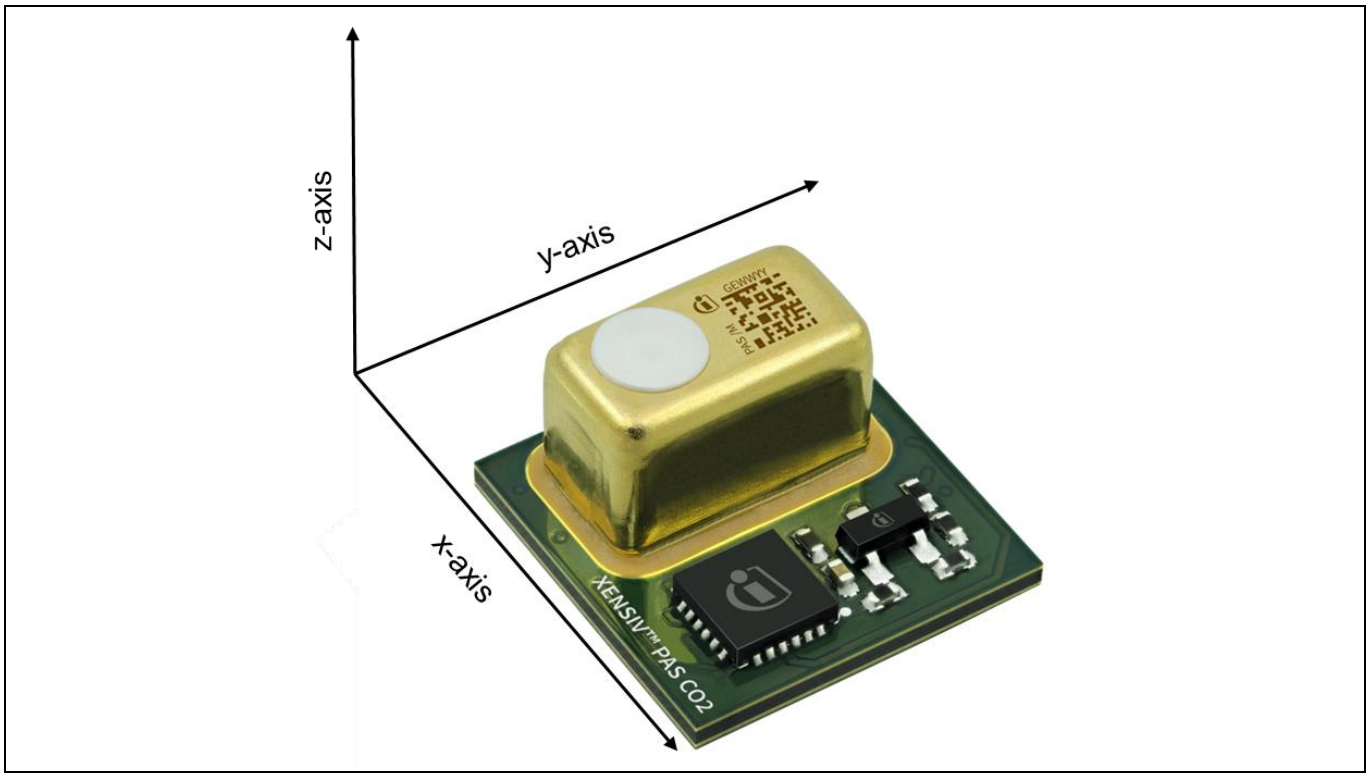

Figure 4 The sensor should be placed in the x-direction of the vibration source

- **Isolation from sunlight:** If the sensor is exposed to sunlight, it may heat up and create a temperature gradient. This temperature gradient may block proper temperature compensation by the sensor, and therefore it is recommended to isolate the sensor from sunlight
- **Non-condensing operation:** The device must be used for non-condensing operation only. Water accumulation near the circuitry may damage the sensor irreparably

An ideal chamber design incorporating the preventive measures mentioned is shown in Figure 5.

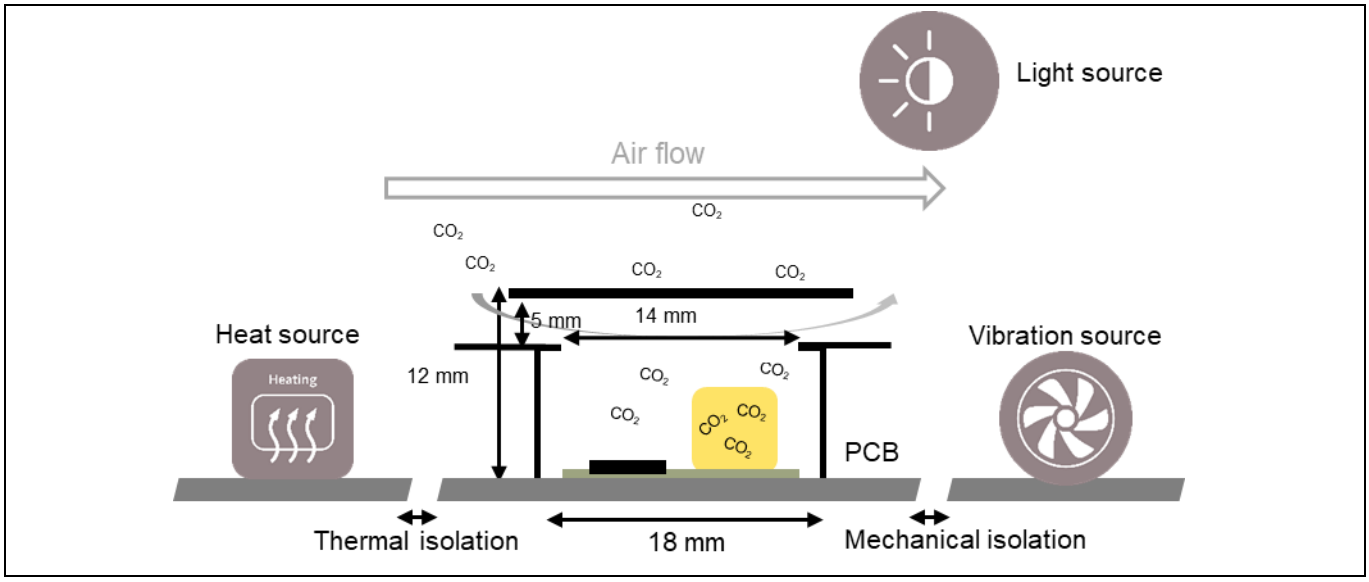

Figure 5 **Preventive measures should be considered when designing the application using XENSIV™ PAS CO2**

3.3 Minimize noise in 12 V supply line

To minimize the noise in the 12 V supply line, a set of decoupling capacitors should be used. Decoupling capacitors act as local electrical energy storage and need time to charge or discharge. Therefore, they oppose quick voltage changes and only pass through the DC component of the signal. As a recommendation, as shown in Figure 6, 47 µF, 100 nF and 10nF should be connected between 12 V and GND to cover a wide noise spectrum in the 12 V line and should be placed as close as possible to the VDD12 pin. Generally, the sensor is robust against supply noise and ripple. The supply can be prepared with cost-efficient components as shown in Figure 6.

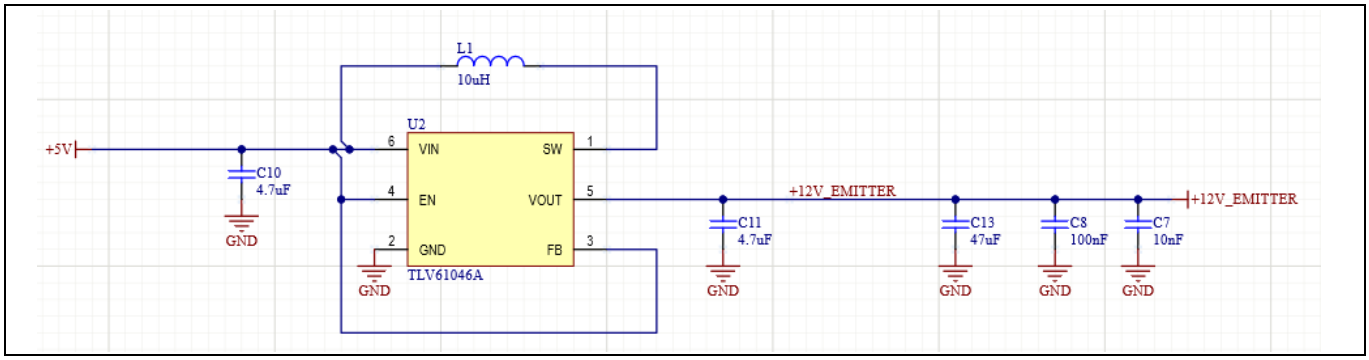

Figure 6 **Recommended circuit to decouple 12 V supply voltage (e.g., PASCOV01)**

3.4 Assembly instructions

XENSIV™ PAS CO2 module is classified as Moisture-Sensitivity Level 3 (MSL 3). The maximum reflow temperature during board assembly must not exceed 245°C, as specified in the IPC/JEDEC J-STD-020E standard.

As shown in Figure 7, Pad 1 to 14 need to be soldered. Pad 1 to 10 need to be assembled as per functionality. Pad 11 and 13 need to be connected to GND. Pad 12 and 14 are not internally connected but must be soldered to maintain mechanical stability. Pad 12 and 14 can be left open or connected to GND. Non-marked smaller pads should be kept open. Further details such as footprint drawing, board assembly guidelines, stencil

recommendation can be found into CO2 product page under Infineon package name 'LG-MLGA-14-1' for PASCOV01, and 'LG-MLGA-14-2' for PASCO2V15.

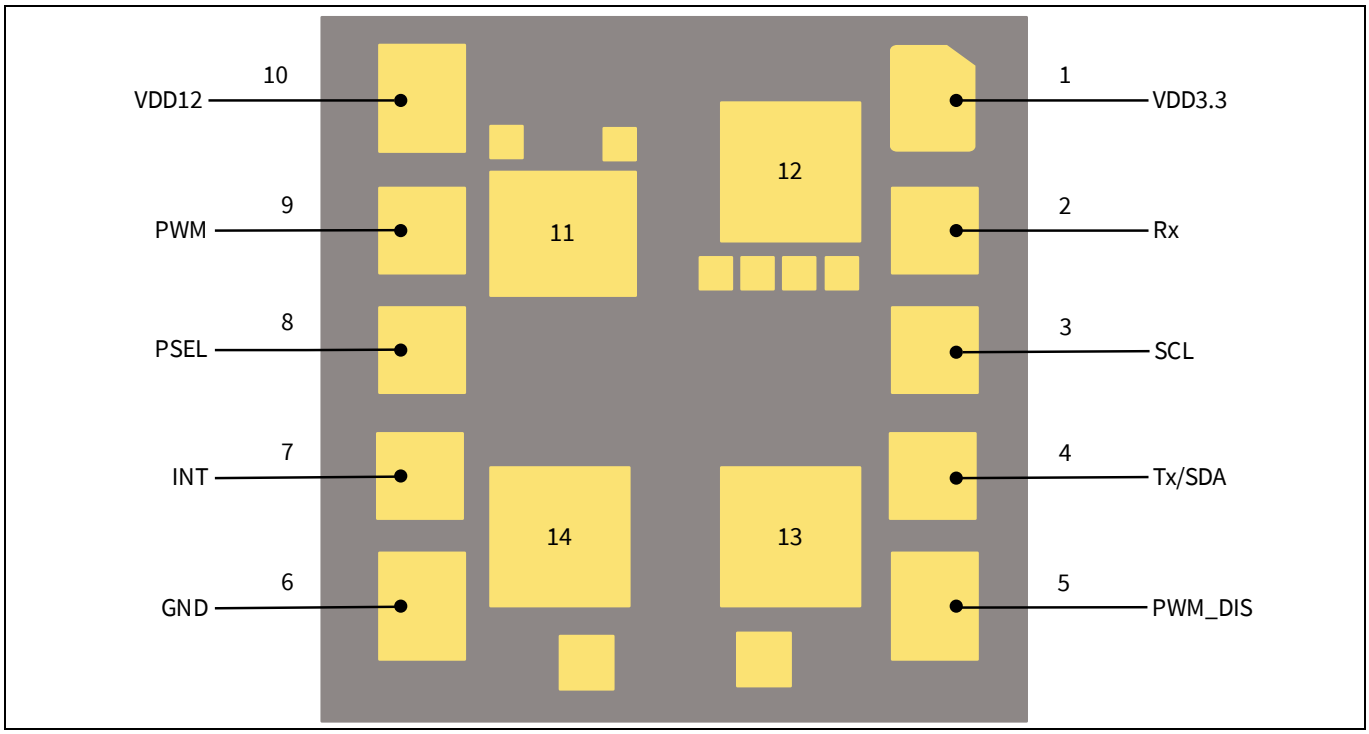

Figure 7 XENSIV™ PAS CO2 pads need to be connected on an application board (e.g., PASCOV01)

Note:

1. *One time reflow is permitted and after assembly rework is not recommended*
2. *Vapor phase soldering may damage the sensor irreversibly*
3. *It is recommended to assemble the module shortly after opening the moisture bag (within 24 hours)*

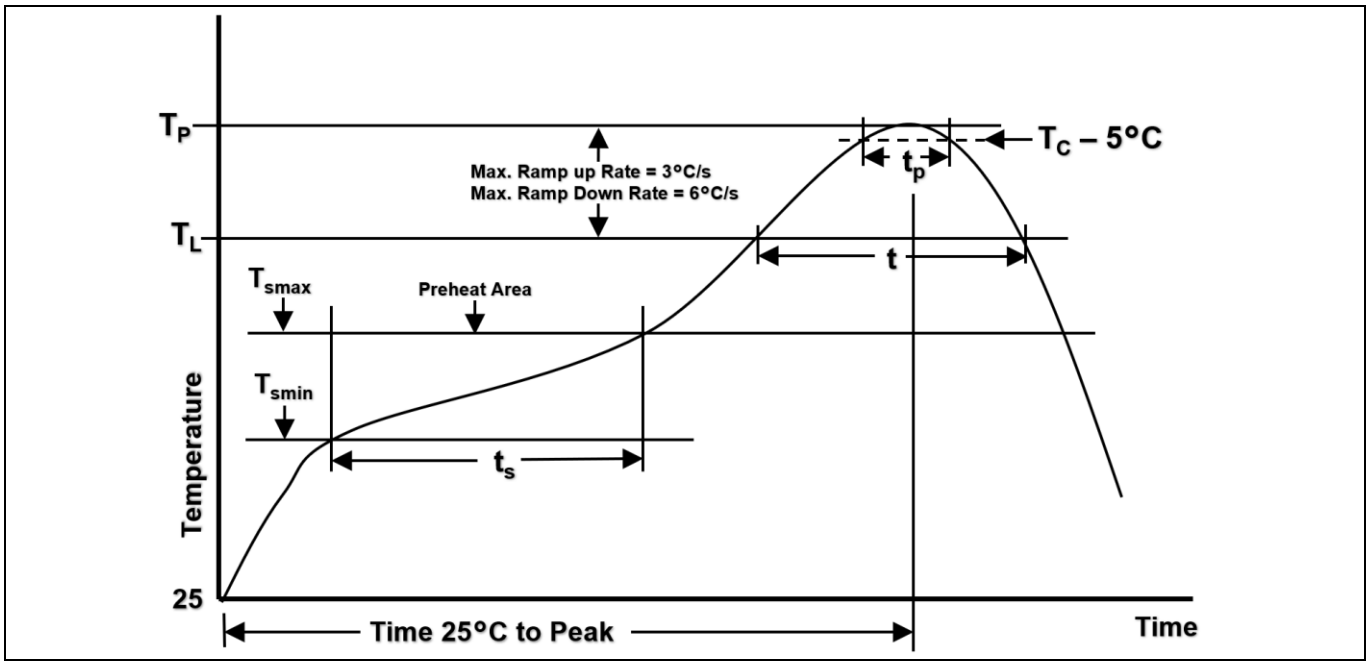

Figure 8 Reflow profile according to JEDEC J-STD-020E

Table 1 Reflow profile according to JEDEC J-STD-020E

Profile Feature	Sn-Pb Eutectic Assembly	Pb-Free Assembly
Preheat/Soak Temperature Min (T_{smin}) Temperature Max (T_{smax}) Time (t_s) from (T_{smin} to T_{smax})	100°C 150°C 60 – 120 seconds	150°C 200°C 60 – 120 seconds
Ramp-up rate (T_L to T_P)	3°C/second max.	3°C/second max.
Liquidous temperature (T_L) Time (t_L) maintained above T_L	183°C 60 – 150 seconds	217°C 60 – 150 seconds
Peak package body temperature (T_P)	245°C	245°C
Time (t_P) within 5°C of the specified classification temperature (T_C)	20 seconds	30 seconds
Ramp-down rate (T_P to T_L)	6°C/second max.	6°C/second max.
Time 25°C to peak temperature	6 minutes max.	8 minutes max.

4 Typical application scenarios

4.1 Influence of acoustic signal within a speaker

PAS technology relies on a high SNR microphone to detect CO2. Therefore, it is a general concern for an end-user that the sensor might be impacted by ambient noise. However, thanks to our robust package, the sensor is acoustically isolated from the surrounding noise. The sensor has been designed in such a way that only CO2 molecules can diffuse within the measurement chamber, while significantly attenuating the surrounding noise. As shown in Figure 9, any position fulfilling the previously discussed prevention recommendation should be sufficient to ensure ideal sensor performance within a speaker. A test has been conducted with the following condition:

- **Ambient condition:** Temperature 25°C, Relative humidity 50%, Pressure 960 hPa
- **Noise level:** Pink noise sweep from 83 dB to 101dB SPL (Sound Pressure Level)

The sensor (PASCO2V01) remained within the specification for the test condition at four different positions of the speaker within the denoise filter enabled.

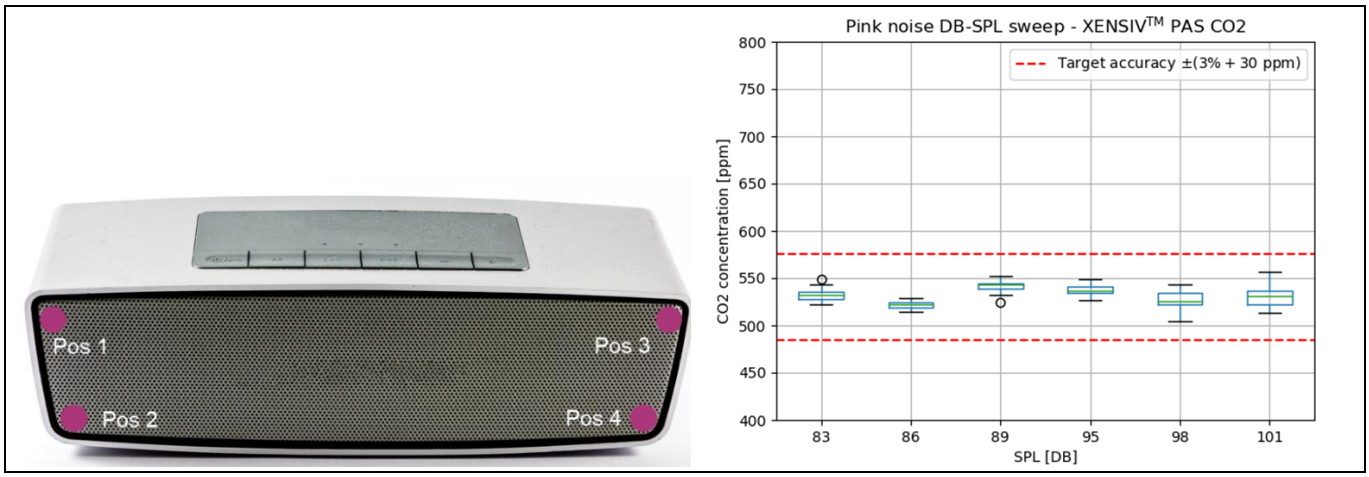

Figure 9 Acoustic robustness of XENSIV™ PAS CO2 sensor (e.g., PASCOV01)

Pink noise is widely present within modern-day music and typically the frequency band is 100 Hz to 10000 Hz. For an analogy, at a subway station or in a disco bar 1m away from the speaker the sound pressure level may reach up to 100 dB. XENSIV™ PAS CO2 sensor output is well within specification even at such a high sound pressure level.

4.2 Influence of vibration within an air purifier

It is highly recommended to isolate the sensor from a vibration source. In typical application scenarios, the vibration may not be a significant concern. As illustrated in Figure 10, three sensors were mounted on a commercially available air purifier. The test results indicate that the sensor remains robust against vibration from the air purifier's fan, even when the denoiser filter is enabled.

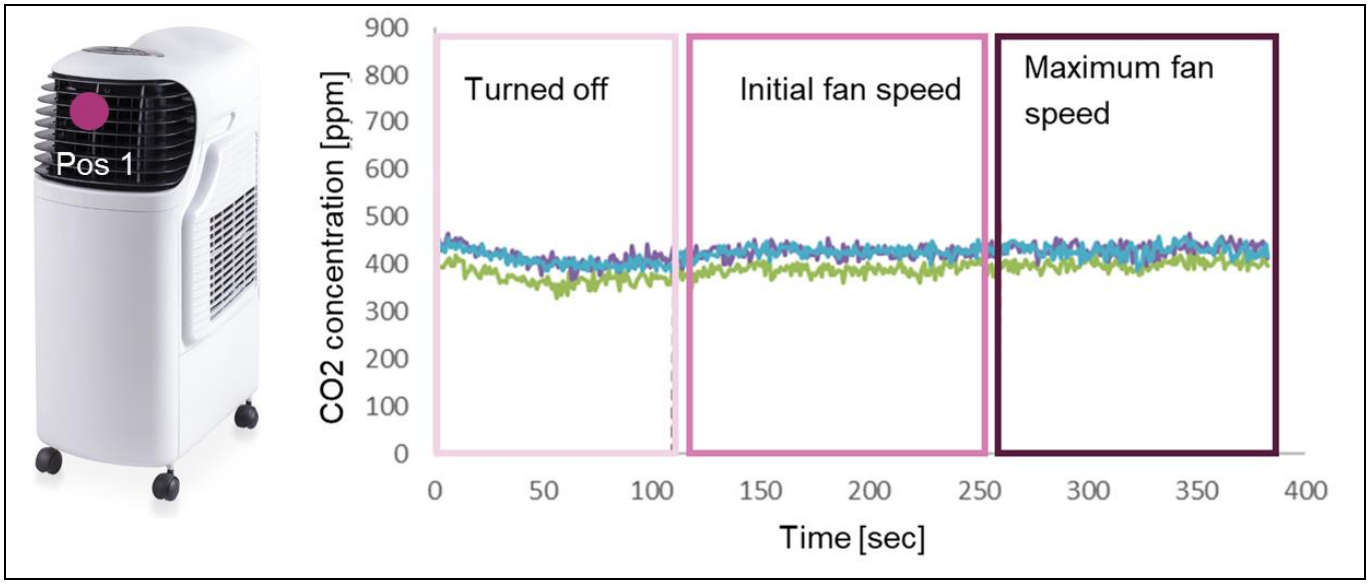

Figure 10 Vibration robustness of XENSIV™ PAS CO2 sensor (e.g., PASCOV01)

4.3 Sensor coverage within an indoor environment

Simulation results show that, regardless of room size, number of people, or sensor location, one sensor is sufficient to cover an entire room.

Application scenario: Meeting room

- Six adults sitting in a meeting room (30 m^2)
- CO2 concentration is monitored at three different locations: the floor (Probe 1), the wall (Probe 2), and the ceiling (Probe 3)

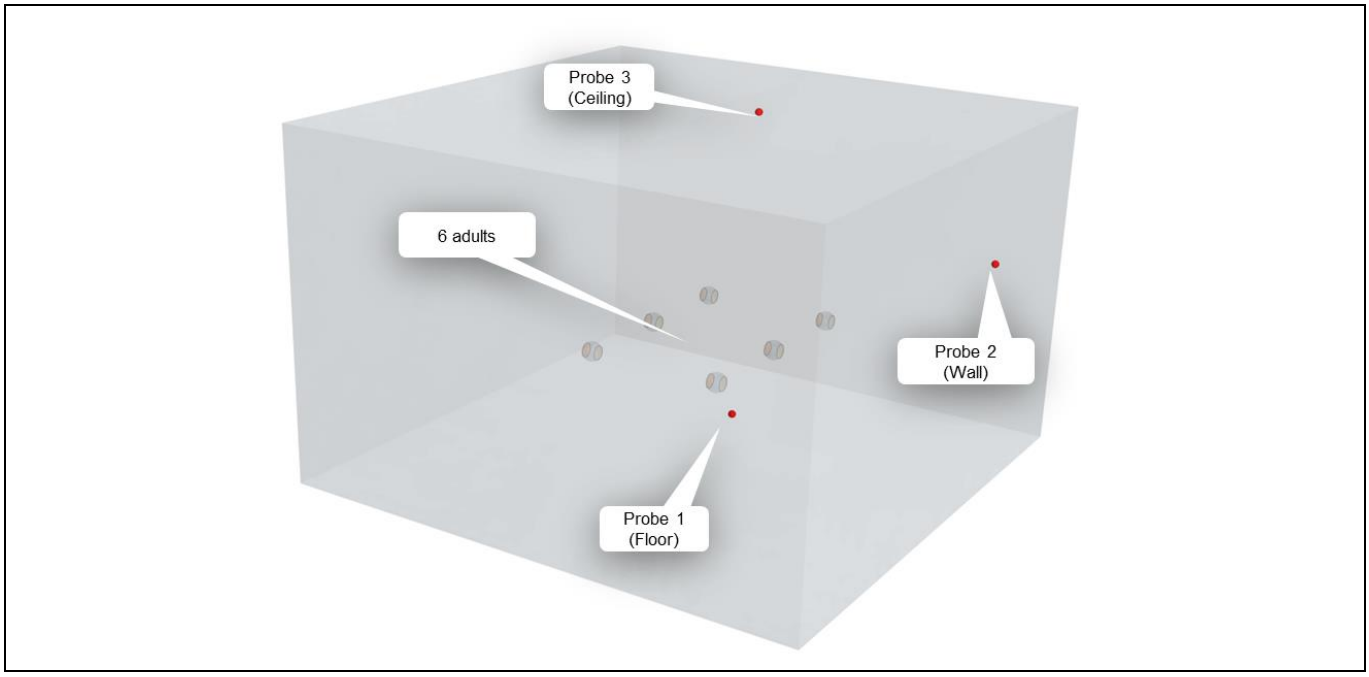

Figure 11 Typical meeting room in an office environment

Typical application scenarios

Assumption:

- Air volume exhaled per human: 8 l/min
- CO2 emission per adult: 900 g/day
- Heat emission per human: 60 W
- Poor ventilation system with limited air exchange

Result:

- The CO2 concentration is found to be similar across different probe locations, with no significant differences observed.

References

[1] Infineon Technologies AG: *XENSIV™ PASCO2V01 gas sensor datasheet*; Available online

[2] Infineon Technologies AG: *XENSIV™ PASCO2V15 gas sensor datasheet*; Available online

Revision history

Document revision	Date	Description of changes
Revision 1.00	2021-06-11	Initial release
Revision 1.10	2022-02-28	Updated Figure 10
Revision 1.20	2022-07-01	Added assembly instructions
Revision 1.30	2025-05-06	Updated template Changed document ID Editorial updates

Trademarks
All referenced product or service names and trademarks are the property of their respective owners.

Edition 2025-05-06

Published by

Infineon Technologies AG

81726 Munich, Germany

© 2025 Infineon Technologies AG. All Rights Reserved.

Do you have a question about this document?

Email: erratum@infineon.com

Document reference

AN213134

Important notice

The information contained in this application note is given as a hint for the implementation of the product only and shall in no event be regarded as a description or warranty of a certain functionality, condition or quality of the product. Before implementation of the product, the recipient of this application note must verify any function and other technical information given herein in the real application. Infineon Technologies hereby disclaims any and all warranties and liabilities of any kind (including without limitation warranties of non-infringement of intellectual property rights of any third party) with respect to any and all information given in this application note.

The data contained in this document is exclusively intended for technically trained staff. It is the responsibility of customer's technical departments to evaluate the suitability of the product for the intended application and the completeness of the product information given in this document with respect to such application.

Warnings

Due to technical requirements products may contain dangerous substances. For information on the types in question please contact your nearest Infineon Technologies office.

Except as otherwise explicitly approved by Infineon Technologies in a written document signed by authorized representatives of Infineon Technologies, Infineon Technologies' products may not be used in any applications where a failure of the product or any consequences of the use thereof can reasonably be expected to result in personal injury.