

Automatic baseline offset correction and forced compensation features of XENSIV™ PAS CO2

Automatic baseline offset correction (ABOC) and forced compensation scheme (FCS).

About this document

XENSIV™ PAS CO2 is an optical system. Like any other optical instrument, due to mechanical stress created by the assembly process, the XENSIV™ PAS CO2 sensor could experience a shift in its characteristics. This materializes into a marginal offset error (typically +/-50ppm) which is normally automatically corrected during operation thanks to the automatic baseline offset correction (ABOC) feature. This means that it is not required to recalibrate the sensor after assembly. If, for specific application use cases, the correction of the offset error is required, the device supports forced compensation scheme (FCS) enabling a fast and cost-effective offset calibration at the customer assembly line.

In this document, the implementation of these schemes will be discussed in detail.

Scope and purpose

The implementation of FCS and ABOC will be discussed for different application scenarios. Depending on the application requirements, either of these two schemes can be implemented.

Intended audience

Application engineers, system engineers and system architects of an application where XENSIV™ PAS CO2 will be used. Additionally, engineers responsible for XENSIV™ PAS CO2 assembly and installation.

Table of contents

About this document.....	1
Table of contents.....	1
1 Offset compensation features of XENSIV™ PAS CO2	2
1.1 Application scenarios using Forced Compensation Scheme (FCS).....	2
1.2 Application scenarios using ABOC.....	2
2 Implementation of FCS and ABOC	3
2.1 Forced compensation scheme.....	3
2.2 Automatic baseline offset correction	4
3 Recommended reference sensor	6
Revision history.....	7

1 Offset compensation features of XENSIV™ PAS CO2

The XENSIV™ PAS CO2 is a real CO₂ sensor that overcomes the size, performance and assembly challenges of existing CO₂ sensor solutions. Designed based on the unique photoacoustic spectroscopy (PAS) concept, the sensor comes in an exceptionally miniaturized optical instrument. Therefore, the sophisticated sensor could show a shift in its characteristics due to stress generated on the light source during the assembly process. This materializes into a marginal offset error (typically +/- 50 ppm) which is normally automatically corrected during operation thanks to the sensor's ABOC feature.

If, for specific application use cases, the correction of the offset error is required, the device supports forced compensation scheme (FCS) enabling a fast and cost-effective offset calibration at the customer assembly line. For both schemes, a reference CO₂ concentration needs to be considered. The reference value can be read from a reference sensor. Alternatively, after assembly, the XENSIV™ PAS CO2 can be exposed to the outside air where the average outdoor air CO₂ concentration can be considered as 400 ppm. In the following section, these two schemes are discussed in detail.

1.1 Application scenarios using Forced Compensation Scheme (FCS)

- **Scenario 1:** Correction of offset error after assembly/reflow

In this scenario FCS is recommended to be implemented at the assembly site. Before evaluating the accuracy of the sensor, it is recommended to perform FCS to minimize the offset shift.

- **Scenario 2:** The application conditions do not fulfill the primary condition of the ABOC scheme

The raw signal of the sensor might drift over time due to aging, and implementing ABOC is the recommended mode of operation to mitigate such a drift. However, for applications where the sensor will not be regularly exposed to a minimum CO₂ baseline concentration during operation, the primary condition of the ABOC scheme is not fulfilled. Therefore, for such an application FCS could be used

1.2 Application scenarios using ABOC

To correct the initial offset after assembly and slow drifts caused by aging during operation, the device supports ABOC. Therefore, for example in an application scenario where the sensor's sampling frequency is one measurement per 60 seconds and generally exposed to outdoor air for at least 30 minutes a week consecutively, ABOC should be implemented. Two possible scenarios are discussed below.

- **Scenario 1:** If the measurement rate is chosen as one measurement in 30 minutes or less, the sensor needs to be exposed to fresh air for at least 30 consecutive minutes within a week for the ABOC to work properly.
- **Scenario 2:** Alternatively, if the measurement rate is chosen as one measurement in more than 30 minutes, then the sensor should be exposed to the fresh air for at least similar to the measurement rate. For example, if the sampling frequency is one measurement per hour, then the sensor needs to be exposed for at least one hour.

Note: Both FCS and ABOC can be used very easily using the Sensor2Go kit via GUI. For further details please, check the user manual of the Sensor2Go kit from this [LINK](#).

2 Implementation of FCS and ABOC

2.1 Forced compensation scheme

Before implementing the FCS, the sensor needs to be exposed to the reference CO₂ concentration for 3 measurement points. Reference CO₂ concentration can be considered in two methods:

- **Method 1:** Expose the sensor to outdoor fresh air and consider the average outdoor CO₂ concentration is 400 ppm.
- **Method 2:** Expose the sensor to a known CO₂ concentration within a sealed chamber. Reference CO₂ concentration needs to be within 350 ppm and 1500 ppm. A recommended reference sensor will be discussed in the next chapter.

Two registers, CALIB_REF_H and CALIB_REF_L, need to be programmed properly to implement the FCS. When FCS is enabled ([MEAS_CFG.BOC_CFG](#) = 10b), the device will use the next 3 measurements to calculate the compensation offset. It is recommended to wait long enough so that the CO₂ concentration is stable in the vicinity of the sensor. The ambient temperature and pressure should also be stable. Therefore, at one measurement per 10 s sampling rate, the device needs to be exposed to the reference concentration for at least 30 s. When the 3 measurement sequences are completed, the device automatically reconfigures itself with the newly computed offset applied to the subsequent CO₂ concentration measurement. The implementation technique of the FCS scheme is summarized in figure 1.

Note: The device's measurement rate must be 1 measurement per 10 s when triggering FCS. After implementing FCS, the ABOC data is reset and the device will automatically switch back to ABOC mode.

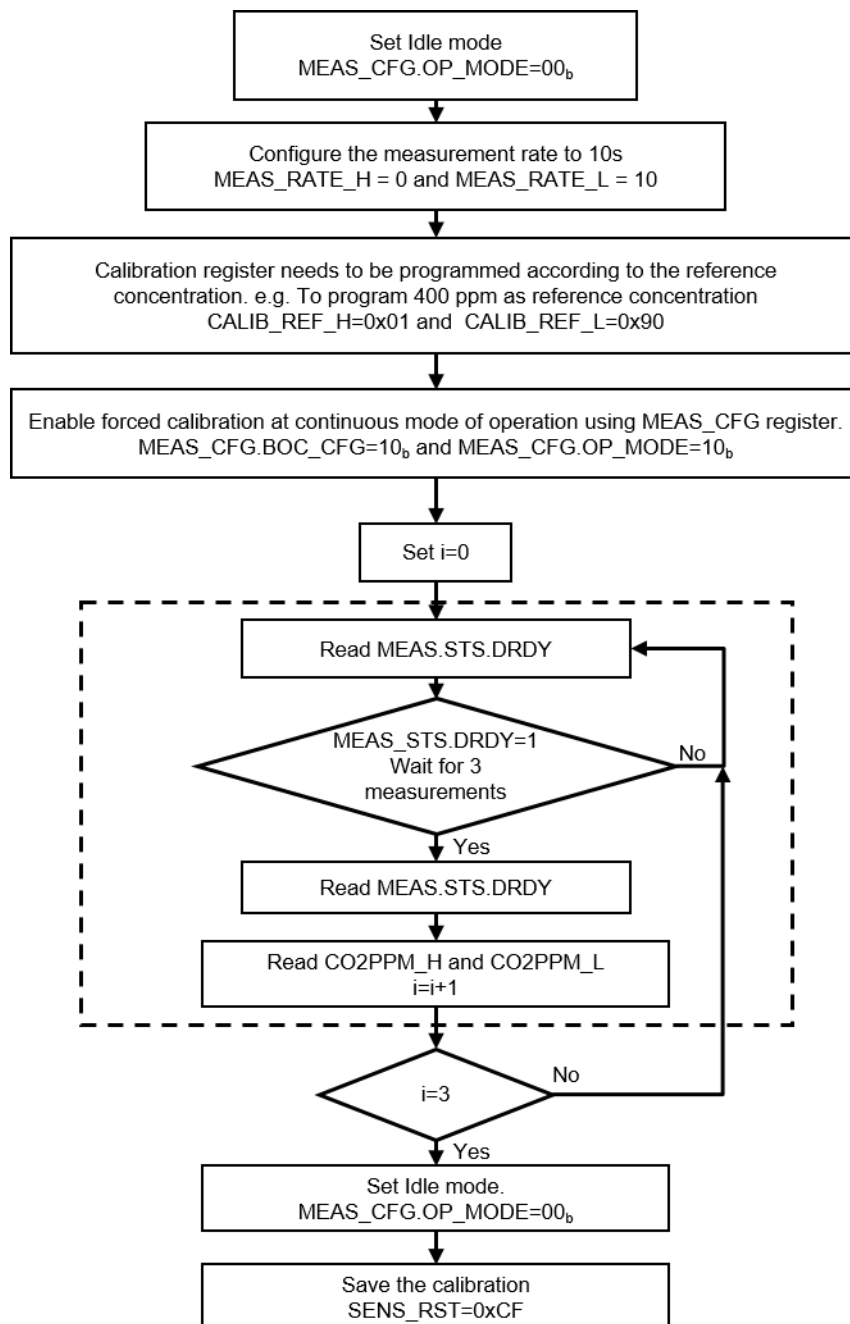


Figure 1 Process flow to implement FCS. 400 ppm has been considered as the reference concentration.

2.2 Automatic baseline offset correction

Per default XENSIV™ PAS CO2 is operating in continuous mode with ABOC enabled. Every week of operation, the device keeps track of the minimum value recorded over that time. The offset to the reference baseline is computed and used to calculate the correction factor to be applied for the week after. The offset update frequency is based on the accumulated operating time of the device and independent of the chosen sampling frequency. However, the time windows for which the device is powered off completely (**VDD3.3** not present) will not be considered. The offset computation scheme assumes that the maximum difference between two correction factors computed consecutively (week to week) remains within **+/-50 ppm**. To ensure proper

Automatic baseline offset correction and forced compensation features of XENSIV™ PAS CO2

Implementation of FCS and ABOC

operation of the ABOC scheme please ensure settings for the relevant scheme have been considered, as discussed in section 1.2. The implementation of the ABOC has been illustrated using the following figure.

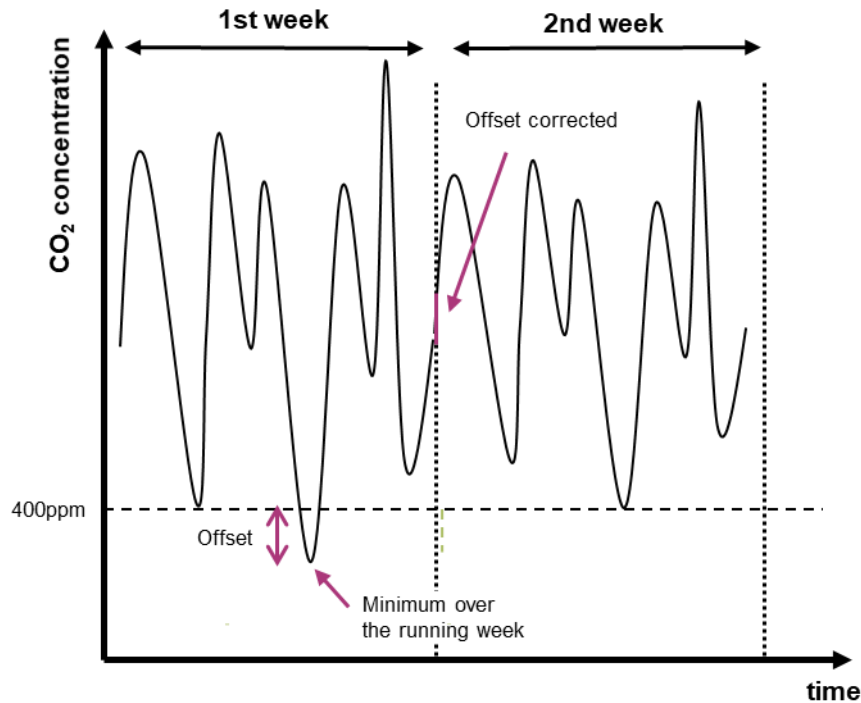


Figure 2 Operation of the ABOC

Note: For the very first ABOC update, the capping assumption (maximum difference between two correction factors computed consecutively, week to week, remains within $\pm 50\text{ppm}$) is not valid. The history of readings required for ABOC algorithm is stored in the non-volatile memory after one hour of continuous operation.

ABOC can only be used with the continuous mode of operation. If automatic baseline compensation is enabled (`MEAS_CFG.BOC_CFG = 01b`), the latest valid computed correction factor is applied to the measured CO₂ concentration value. The offset correction is calculated based on the reference value programmed in register `CALIB_REF_H` and `CALIB_REF_L`.

Note: The default reference CO₂ concentration is considered to be 400 ppm. The reference value should only be adjusted for a very specific application scenario.

3 Recommended reference sensor

Vaisala GMP343 is recommended as the reference CO₂ sensor. Further details of this product can be found on the product [page](#).

Revision history

Revision history

Document version	Date of release	Description of changes
V1.0	02.06.2021	Creation
V1.1	23.08.2021	Published
V1.2	15.12.2021	Update to Forced Compensation Scheme, new Title
V1.3	01.07.2022	Minor changes and rephrasing

Trademarks

All referenced product or service names and trademarks are the property of their respective owners.

Edition 2022-07-01

Published by

Infineon Technologies AG

81726 Munich, Germany

© 2022 Infineon Technologies AG.

All Rights Reserved.

Do you have a question about this document?

Email: erratum@infineon.com

Document reference

AN_2106_PL38_2106_095830

IMPORTANT NOTICE

The information contained in this user manual is given as a hint for the implementation of the product only and shall in no event be regarded as a description or warranty of a certain functionality, condition or quality of the product. Before implementation of the product, the recipient of this user manual must verify any function and other technical information given herein in the real application. Infineon Technologies hereby disclaims any and all warranties and liabilities of any kind (including without limitation warranties of non-infringement of intellectual property rights of any third party) with respect to any and all information given in this user manual.

The data contained in this document is exclusively intended for technically trained staff. It is the responsibility of customer's technical departments to evaluate the suitability of the product for the intended application and the completeness of the product information given in this document with respect to such application.

For further information on the product, technology, delivery terms and conditions and prices please contact your nearest Infineon Technologies office (www.infineon.com).

WARNINGS

Due to technical requirements products may contain dangerous substances. For information on the types in question please contact your nearest Infineon Technologies office.

Except as otherwise explicitly approved by Infineon Technologies in a written document signed by authorized representatives of Infineon Technologies, Infineon Technologies' products may not be used in any applications where a failure of the product or any consequences of the use thereof can reasonably be expected to result in personal injury.