OneEye_DAS_Oscilloscope_1 for KIT_AURIX_TC367_TFT Oscilloscope over DAS using OneEye

AURIX[™] TC3xx Microcontroller Training V1.0.0



Please read the Important Notice and Warnings at the end of this document



Demonstrate how to implement the OneEye oscilloscope over the DAS interface.

After configuring the OneEye DAS interface, a OneEye oscilloscope is created with two signals. The signals are updated and sampled every millisecond. OneEye is used to visualize the signal values.



Introduction


- OneEye is a GUI that enables the creation of interactive Graphical User Interface. Graphical elements can be drag from a toolbox and drop onto the GUI. The behavior of the created GUI can be customized. Different communication interfaces like UART, Ethernet, CAN, DAS can be used to interact with the embedded system
- The DAS (Device Access Server) can be used in line with Infineon Microcontroller Starter Kits, Application Kits and DAP MiniWiggler to access the micro controller resources
- Recommendation: It is recommended to go through some of the basic tutorials listed in the help embedded in OneEye (Menu: Help -> OneEye help). This enables a quicker rampup in the OneEye concept and ensure a nice journey with OneEye



Hardware setup

This code example has been developed for the board KIT_A2G_TC367_5V_TFT.

The board should be connected to the PC through the USB port 1

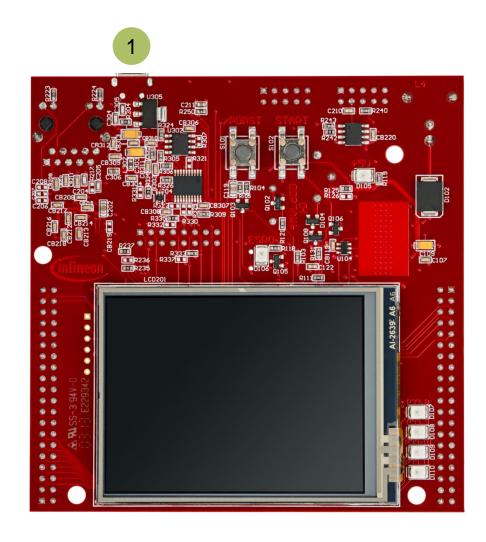



Implementation - AURIX

Configuring the OneEye Oscilloscope

A OneEye oscilloscope (*Ifx_Osci*) is a special object that is recognized by OneEye. It enables streaming of data and controls the oscilloscope state.

The OneEye oscilloscope is initialized with *lfx_Osci_init()*.

The *autoAddChannels* parameter enables to automatically add channels for each created oscilloscope signal. The sample period (*samplePeriod*) is set to 1ms and provides OneEye information about sample timing. The *triggerMode* is set to automatic, note that this value can be changed from the OneEye oscilloscope interface later.

The **lfx_Osci.h** file can be found in the Libraries\OneEye directory.

Adding signals to the oscilloscope

Oscilloscope signals are mainly pointers that the oscilloscope can use for data sampling. The signals are added using *lfx_Osci_addSignal()*. The function takes as parameter the signal **name** displayed by the oscilloscope, the signal **type** which informs the oscilloscope how to read the pointer value and a **source** pointer to the data. The last parameter corresponds to the **q format** used in case of fix point data, or 0 if not used.

Starting the oscilloscope

The oscilloscope is started with *lfx_Osci_start()*.



Implementation - AURIX

Configuring the signal generator

A signal generator is used to provide the user with some value to read / write. The signal generator does nothing more that incrementing two signals, *signalA* and *signalB*, stored in the structure *g_signalGenerator* up to a maximum value before resetting them.

The initialization of the signal generator is done with *initSignals()*.

Running the signal generator and the oscilloscope

The signal generator is executed in the background loop every 1ms with *computeSignals()*. For that a **deadline** variable is initialized with *getDeadLine()* and periodically updated with *addTTime()* to obtain the 1ms period.


The oscilloscope is run in the same background loop with *lfx_Osci_step()*. This function handles the triggering, and sampling of data.

Note: the call to *lfx_Osci_step()* can be moved to an interrupt service routine if required by the application use case.



Run and Test

- After code compilation, flash the device using the Flash button 1 to ensure that the program is running on the device
- For this training, the OneEye application is required for visualizing the values. OneEye can be opened inside the AURIX[™] Development Studio using the following icon:

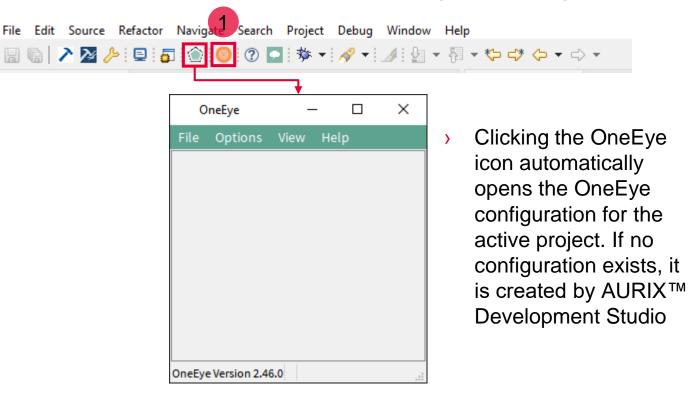



In this training, the OneEye configuration is provided inside the Libraries folder. The following steps are needed to configure the oscilloscope from a brand-new configuration.

Setup OneEye for editing

Select the OneEye menu "**Options -> Edit mode**" (if not already checked) to enable the edit mode. Select the OneEye menu "**View -> Browser box**", "**View -> Property box**", "**View -> Tool box**" (if not already checked) to display the browser, property box, and tool box.

OneEye		-	
File Options View Help			
ool box	₽×	Property box	
	^		
Bar Gauge			
Check Box			
Check Box			
(\checkmark)			
Clock Gauge			
opt V Combo Box			
(\bullet)			
Dial			
+			
Graph			
+			
Graph Channel			
Group	*		
<	>		
rowser box	& ×		
All	~		
	le		
signals layout			
> interface interface.			
configuration			
debugBox			
<	>		



Configuring the DAS interface

When the OneEye configuration is created by ADS, it is already setup with a DAS interface. Select the DAS interface in the Browser box 1.

Notice the "system-key" {ADS} that enables the connection to the device in parallel with the ADS debugger.



Create a debug box to get access to variables from the .elf file

A debugBox item is already setup by default when ADS creates the OneEye configuration, preconfigured with the project .elf file path.

Select the DAS interface in the Browser box <

Set the id property to "elf", which enables to group variables into the signal tree later.

Note: this value is not set by default by ADS.

	₽×		Property box	
Bar Gauge	^		Debug box: elf-path	debugBox
Check Box			watches	lloscope_KIT_TC375_L
Clock Gauge				
Combo Box				
Dial				
Graph				
Graph Channel				
Group	,			
Group box				
<	>			
< Browser box	> & ×			
k k k k k k k k k k k k k k k k k k k	> & x			
C Browser box All Path Object signals	> & ×			
All Path Object signals layout interface interface.	> & x			
All Path Object signals layout	> & x		com-interface-id title	das-itf



Open the debug box viewer and connect to the device

Select the OneEye menu "**View -> Debug box viewer**" (if not already checked) to display the debug box. Select the debug box with the id "(elf)" 1 if not yet selected by default. Note that the debug box enables the selection of the .elf file to be used to get information about the variables.

The **Filter** field 2, enables to filter variables by name. E.g. in this example, entering "g_" will filter for global variables.

To enable the connection with the microcontroller and have read / write access to variables, check the "DAS connection status" box 3.

bug box viewer				
lf) 1				
space/OneEye_DAS_Oscilloscop	e_KIT_TC375_LK/Libraries/\De	bug\OneEye_DAS_Oscilloscope_KIT_TC375_LK.elf	Load ELF file Rel	load ELF file Clear
DAS connection status: 🗹 C	vcle Time: 0007 ms			
DAS connection status: Filter: g_ Name	2 Size	Name	Value	Address



Create signals for signal generator input parameters

In the debug box, search for the *g_signalGenerator* variable, right click on it and select "Add watch on: *g_signalGenerator*". The watch should appear on the right side of the debug box. Watches are periodically polled for new values on the microcontroller.

Expand the **g_signalGenerator** item on the right and right-click on the **max** and **increment** variables to create two signals with the option "Create signal for: ..."

Debug box viewer					×	
(elf)					~	
rix_examples_ads/workspace/OneEye_DAS_Quickstart_KIT_TC375_LK/Libraries/\Debug\O	neEye_DAS_Quickstart_KIT_TC375_LK.e	elf L	oad ELF file Reload	ELF file C	Clear	
Filter: g_			Browser box			x
Name Size g_signalGenerator 16 P_00US00CVP00 4	Name Image: signal Generator Image: signal Generator Image: signal Generator	Val -	All			~
g_cpusyncevent 4	max	0	Path ❤ signals		Object	Title
	✓ output	-	✓ elf		group	
	signalA	0	g_oscil)as	char	g_osciDas
	signalB	0		alGenerator	group	g_signalGenerator
			Ƴ inp		group	input
				max	float	max
The created signa	Is should appear in		layout	increment	float	increment
the browser box u "signals.elf" group	interface configuration debugBox		interface.			
			<			>



Create signals for the oscilloscope

In the debug box, search for the *g_osciDas* variable, right click on it and select "**Create oscilloscope watch on:** *g_osciDas*". The watch should appear on the right side of the debug box 1. Watches are periodically polled for new values on the microcontroller.


A signal is also automatically created to access the oscilloscope 2.

ebug box viewer								x
(elf)								\sim
pace/OneEye_DAS_Oscilloscop		.\Debug\OneEye_DAS_(Oscilloscope_KIT_TC375_LK.elf	Load ELF file	e Reload E	LF file	Clear	
Filter:	rcle Time: 0007 ms			Browser box				
Name g_signalGenerator g_cpuSyncEvent	Size 16 4		Name Image: g_signalGenerator g_osciDas	Path V signals		Object	Title	
g_osciDas	21268			✓ g_si	sciDas ignalGenerator input	char group group	2 g_osciDa g_signal(input	s Generator
					max increment	float float	max	t
		-	should appear in er the "signals.elf"	layout > interface configuration debugBox	on	interface.	_	>



Create edit fields for the generator input parameters

Drag and drop the signals **elf.g_signalGenerator.input.max** and **elf.g_signalGenerator.input.increment** from the browser box onto the layout to create default widget for them.

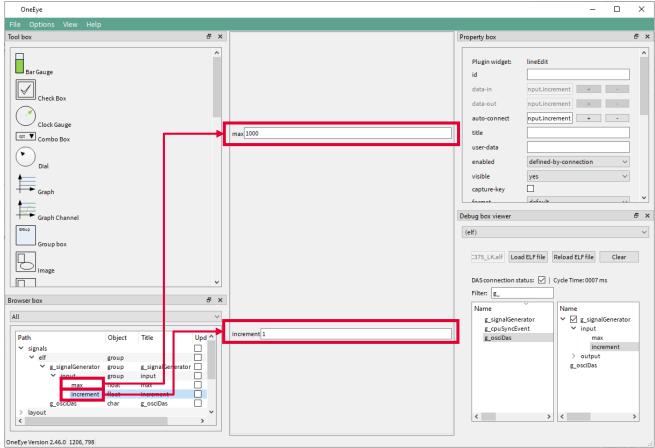



Create the oscilloscope widget

Drag and drop the **oscilloscope** widget from the toolbox onto the layout, set the oscilloscope properties **data-in** and **data-out** to **elf.g_osciDas**. Set the **protocol-type** property to **ProtocolDma**.

OneEye		- 🗆 ×
File Options View Help		
Tool box & ×	max 1000	Property box & X
Tool box B ImageBuffer 'rec Logger Logger Channel Mux-Demux 'rec Named Pipe Client 'rec Oscilloscope Oscilloscope Channel ter Plain Text Edit Path Object Title Upd ^ ' g_ignalGenerator ' group ' gignalGenerator '' input group '' input '' max	max 1000 increment Image: Control g_osciDas Control Control Refresh State Run Triggered Buffer depth 512 Sampling interval Image: Control Time/Div 12/Div Sampling period (s) 0.001 Trigger Single mode Single mode Single Trigger mode Automatic Slope Rising edge Channel CHO: Signal A Level 0	Plugin widget: oscilloscope id
increment float increment i g_osciDas char g_osciDas v > layout v	X: 1s/Div 2.66129 s Control Channel Save Info Hide	g_signalGenerator g_cpuSyncEvent < osciDas > < state="background-color: white;">
OneEye Version 2.46.0 1496, 798		



Test the oscilloscope

In the oscilloscope Channel tab, click on the Channel button **1** and check the **visible** check box for both **CH0: Signal A** and **CH1: Signal B** to display the two channels.

Set the Unit per div Y to 200 for both CH0: Signal A and CH1: Signal B.

Select the Pen color red for CH0: Signal A and blue for CH1: Signal B.

The values for **signalA** and **signalB** should be changing in the oscilloscope, if it is not the case check that the "**DAS connection status**" is checked in the debug box viewer.

One can change the **max** and **increment** values to change the generator behaviour.

OneEye	– 🗆 X
File Options View Help	
max 1000 increment 10 g_osciDas	
D: Signal A Y: 200 Div Value: 100 1: Signal B Y: 200 Div Value: 540	Channel Channel CHO: Signal A Signal Signal A Visible Offset X 0 Offset Y 0 Unit per div Y 200 Pen color red Pen width 1 1
X: 0.0512 s/Div 0.001701 s	Control Channel Save Info Hide
DneEye Version 2.46.0 639, 553	




Test the oscilloscope

The oscilloscope Control tab provides configuration for the trigger and information about the oscilloscope state (armed, triggered, uploading).

Click on the Control button 1 and set the **Time/Div** value to **Zoom All** to configure the horizontal scale to use the full screen of the oscilloscope window.

The **Buffer depth**, configures the oscilloscope buffer depth, here 512 points are used to fill the buffer. This value can be changed within the limit set by the software.

The **Sampling interval** provides the oscilloscope the information whether to sample at each interval (1) or not (>1)

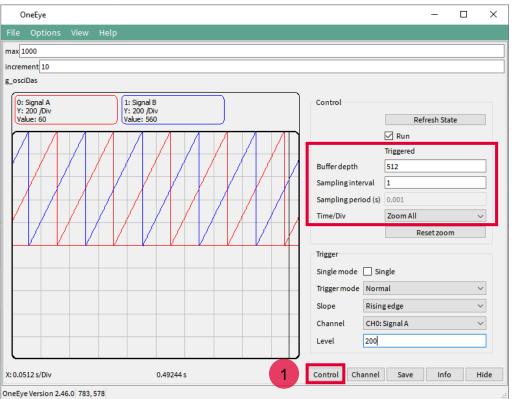



The final configuration should look like the following:

OneEye			-	o x
File Options View Help				
Tool box 🗗 🗙	max 1000		Property box	8×
·	max 1000 increment 1 g_osciDas	Control Refresh State Run Triggered Buffer depth Sampling interval Sampling period (s) Time/Div Reset zoom	Plugin widget: oscilloscope id	-
Plain Text Edit Browser box Browser box Øreining and the second s	X: 0.0512 s/Div 0.00825806 s	Trigger Single mode Single Trigger mode Automatic Slope Rising edge Channel CH0: Signal A Level 0 Control Channel Save Info Hide	protocol-type ProtocolDma dma-refresh-period 100 division-y 10 Debug box viewer (elf)	Clear



Advanced options

Advanced configuration can be added to the file *lfx_Cfg.h* to tune the oscilloscope capabilities, this includes:

- IFX_OSCI_CFG_MAX_NUM_OF_SIGNALS: the maximum number of signals that can be declared by the user
- > IFX OSCI CFG MAX NUM OF CHANNELS: the maximum number of channels that can be buffered
- > IFX_OSCI_CFG_NUM_OF_SAMPLES: the maximum number of sample per channel

Note that the memory used by the oscilloscope is mainly defined by IFX_OSCI_CFG_MAX_NUM_OF_CHANNELS * IFX_OSCI_CFG_NUM_OF_SAMPLES * 4

Default values for the above mentioned macros are provided in *Library/OneEye/Ifx_Osci_Cfg.h*.

References

>













- https://www.infineon.com/aurixdevelopmentstudio
- Use the *"Import…"* function to get access to more code examples. >
- More code examples can be found on the GIT repository: >
- https://github.com/Infineon/AURIX code examples >
- For additional trainings, visit our webpage: >
- https://www.infineon.com/aurix-expert-training >
- For questions and support, use the AURIX[™] Forum: >
- https://www.infineonforums.com/forums/13-Aurix-Forum >

Trademarks

All referenced product or service names and trademarks are the property of their respective owners.



Edition 2022-03 Published by Infineon Technologies AG 81726 Munich, Germany

© 2021 Infineon Technologies AG. All Rights Reserved.

Do you have a question about this document? Email: <u>erratum@infineon.com</u>

Document reference OneEye_DAS_Oscilloscope_1 _KIT_TC367_TFT

IMPORTANT NOTICE

The information given in this document shall in no event be regarded as a guarantee of conditions or characteristics ("Beschaffenheitsgarantie").

With respect to any examples, hints or any typical values stated herein and/or any information regarding the application of the product, Infineon Technologies hereby disclaims any and all warranties and liabilities of any kind, including without limitation warranties of non-infringement of intellectual property rights of any third party.

In addition, any information given in this document is subject to customer's compliance with its obligations stated in this document and any applicable legal requirements, norms and standards concerning customer's products and any use of the product of Infineon Technologies in customer's applications.

The data contained in this document is exclusively intended for technically trained staff. It is the responsibility of customer's technical departments to evaluate the suitability of the product for the intended application and the completeness of the product information given in this document with respect to such application. For further information on the product, technology, delivery terms and conditions and prices please contact your nearest Infineon Technologies office (www.infineon.com).

WARNINGS

Due to technical requirements products may contain dangerous substances. For information on the types in question please contact your nearest Infineon Technologies office.

Except as otherwise explicitly approved by Infineon Technologies in a written document signed by authorized representatives of Infineon Technologies, Infineon Technologies' products may not be used in any applications where a failure of the product or any consequences of the use thereof can reasonably be expected to result in personal injury.